

Neximatic

Innovative Device Connectivity

Installation Guide Philips MP70 (MIB) GE Avance (Cable Assembly 57)



Warning

Each package contains specific materials for the installation in this room.

A label is affixed on this page and it has the information about this room.

Please review the label before installation.

Read the entire instruction guide before starting the installation.

Installation should be performed by an IT, a Bio Tech or a person with knowledge of IT and medical devices.

Some installation may require additional component from the medical device manufacturer.

If there is any question or if there is any unexpected issue, please stop immediately, revert any setting and contact support. Failure to do so may damage the Nexi and/or any medical device.

Package Contents

Item	Description
Nexi	The Nexi communicates with the medical devices and stream medical data to an HER. The Nexi is pre-configured for the medical devices for this room The Nexi is pre-configured for the networking setting for this facility The Nexi can be re-configured for other medical devices when it is connected to the Internet
Cable Assembly	This cable assembly is specific for the medical devices in this room DO NOT DISASSEMBLE THE CABLE ASSEMBLY
Power Supply	This power supply is compatible to the Nexi DO NOT USE OTHER POWER SUPPLY UNLESS ADVISED
Velcro Strips	Use to mount the Nexi
Optional Mount	The package may contain additional mount equipment
Optional QR Tag	Some implementation may include a QR Tag

Installation Procedure

Pre-installation

- Check label for this package to ensure it is for the corresponding room.
- Ensure any necessary tools are available.

Installation

- Nexi: Review the features and ports of the Nexi.
- Medical Devices: Identify the medical devices.
- Power and Mount: Find a suitable mount location and power source.
- Cabling: Connect the cable between medical devices and the Nexi.
- Configuration: Set the medical devices according to instruction.
- Optional QR Code: Affix the QR Code in the front for scanning.

Testing

- Different generations of the Nexis have different test procedure.
- Please following the Test Section for more information.

Post-installation management

- Use wire ties to secure the cable assembly and power cord with enough slack
- If the Nexi is equipped with a cord clip, clip the power cord through it.

Items required for installation

Please have the following ready for an installation

- Wire ties
- Scissors
- Labels
- Screw drivers (Philips)

Nexi: Nexi-N6



Power, * USB and Ethernet

* Depending on the configuration, USB may be used for medical device interfacing.

Nexi-N6 Specification	
Model	Nexi-N6
Operation Voltage	12V DC
Maximum current consumption	1.5A
Operation temperature	25C, in-door only
Operation humidity	5-95%
Interfaces	4 USB ports 1 Ethernet port
Medical Device Interfaces	2 Serial interfaces 1 Ethernet interface
Indicator	Power Internet Service Data Transmission Issue

Medical Device Interfaces

Nexi Name is a globally unique number.

Nexi Name must be provided when contacting support.

Power Source and Mount Location (Anesthesia Machine)

The Nexi should use the power outlet available on the anesthesia machine


Assess the power cord and cabling to the medical devices to find a suitable mount location of the Nexi

- Location should provide enough slack for the power cord and the cabling
- Location should not obstruct any instrument
- Location should provide a clear view of the Nexi, its label and lights

Suggestion of a mount location

On top of the anesthesia machine

At the back of the anesthesia machine

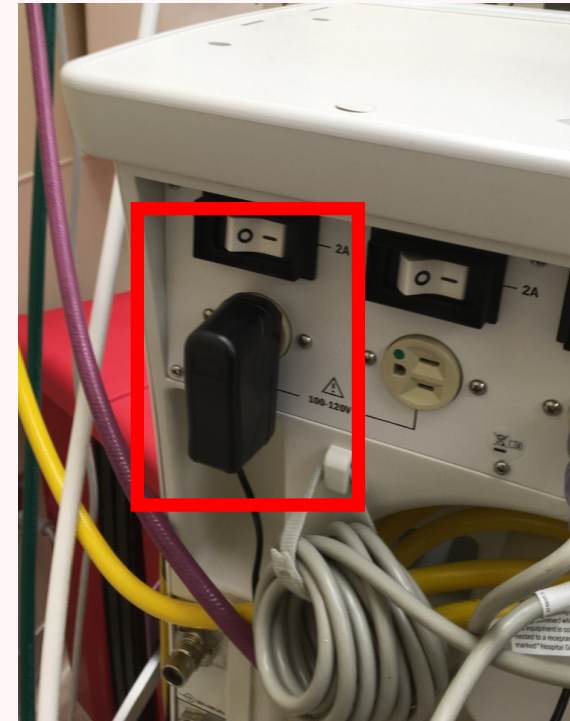


Power Source and Mount Location (Wall Mount)

The Nexi should use the nearest power outlet

The Nexi should be mounted on the wall using Velcro and the mount

- Location should provide enough slack for the power cord and the cabling
- Location should not obstruct any instrument
- Location should provide a clear view of the Nexi, its label and lights

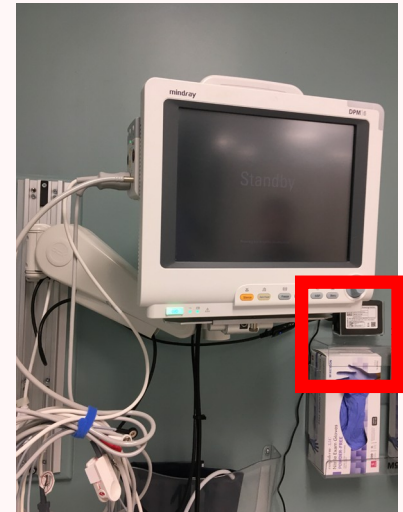

Power Source and Mount Location (Wheeler)

A medical grade power outlet should be mounted on the wheeler

Both the Nexi and the medical device should be connected to the mounted power outlet

The Nexi should be mounted on the medical device

- Location should provide enough slack for the power cord and the cabling
- Location should not obstruct any instrument
- Location should provide a clear view of the Nexi, its label and lights



Medical Device: Philips MP70



Medical Device: GE Avance



Cable: Cable Assembly 57



The cable assembly consists of a Dual-USB cable with 2 ends.

The Serial ends are numbered: #1 and #2.

A Custom Cable C is attached to Serial #1.


A Custom Cable A is attached to Serial #2.

DO NOT DISASSEMBLE.

Cabling: Philips MP70 (MIB)

MP60/MP70

Right side of monitor (MP60/70)

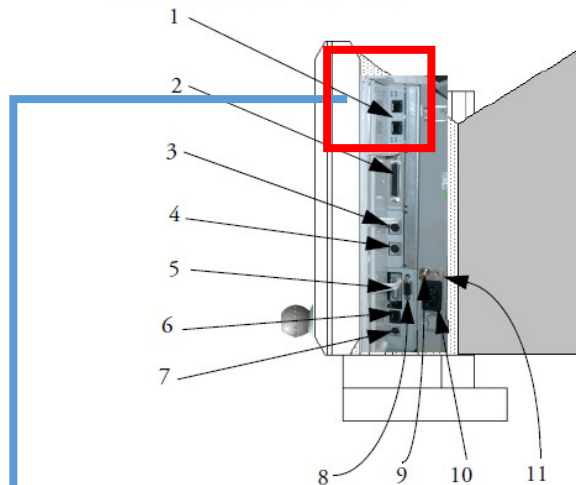

1 Serial/MIB (RS232) connectors (optional), type RJ45

2 Parallel printer connector

3 Keyboard connector

4 Mouse/trackball connector

5 Main measurement link (MSL)

6 Wired network connector

7 Wireless network connector




8 Analog video out connector

9 Equipotential ground connector



10 AC power input

11 Protective earth screw hole

- There are 2 ports.
- Choose a port that has a lit Yellow Arrow Out LED
- If there is no lit Yellow Arrow Out LED, follow the steps in MP70 Configuration

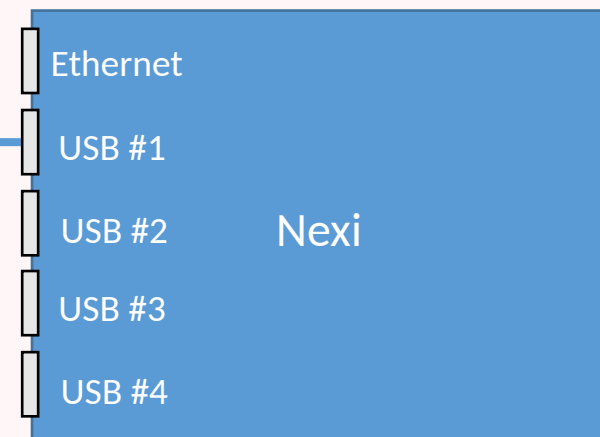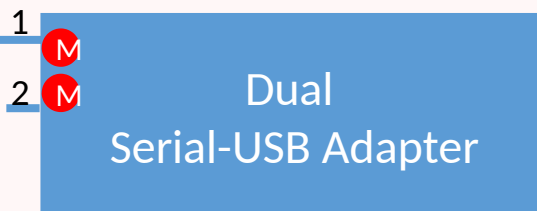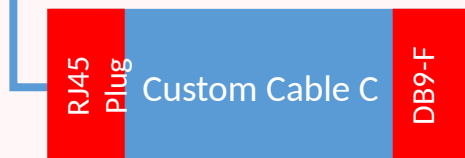


Cabling: GE Avance

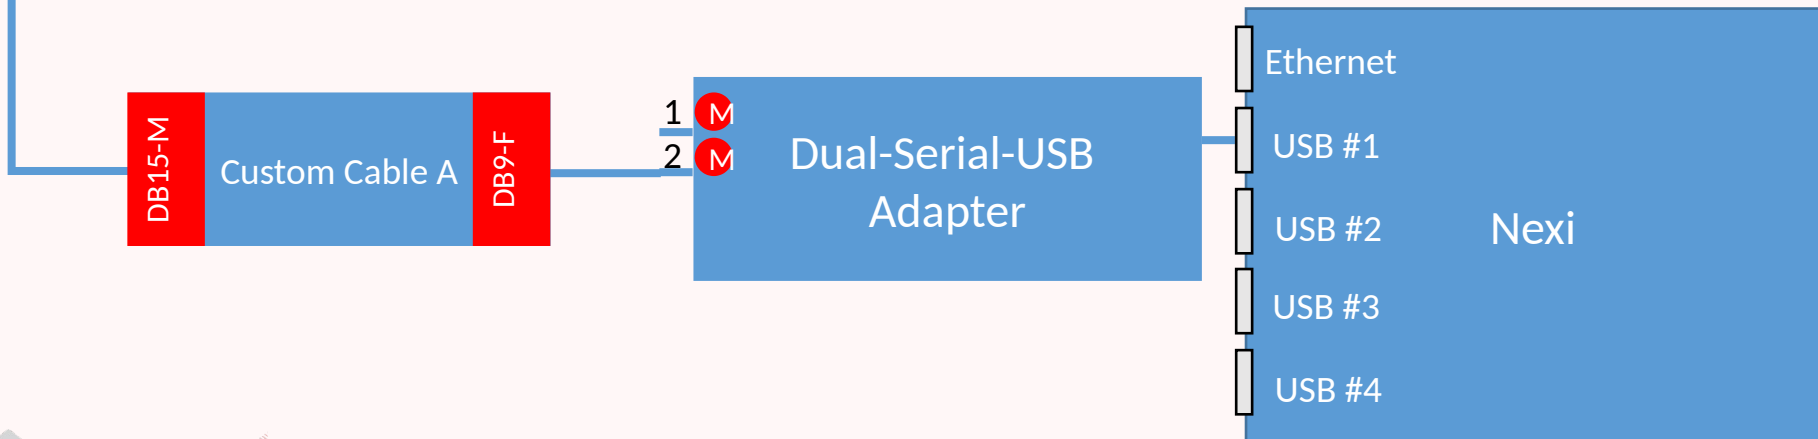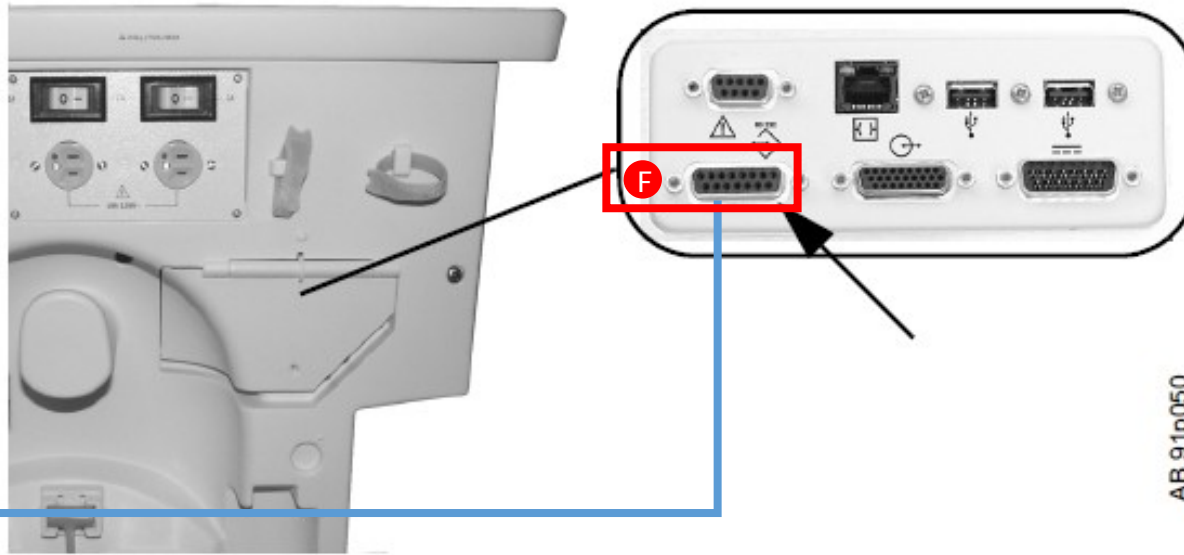

Configuration: Philips MP70 (MIB)


- Determine which MIB port you are using
 - The interface is 04
 - There are "a" and "b"
 - The picture shows a 04b connection
- LEDs on MIB ports
 - Note there are 2 LEDs per MIB
 - We need to set the port so that the Yellow Arrow Out

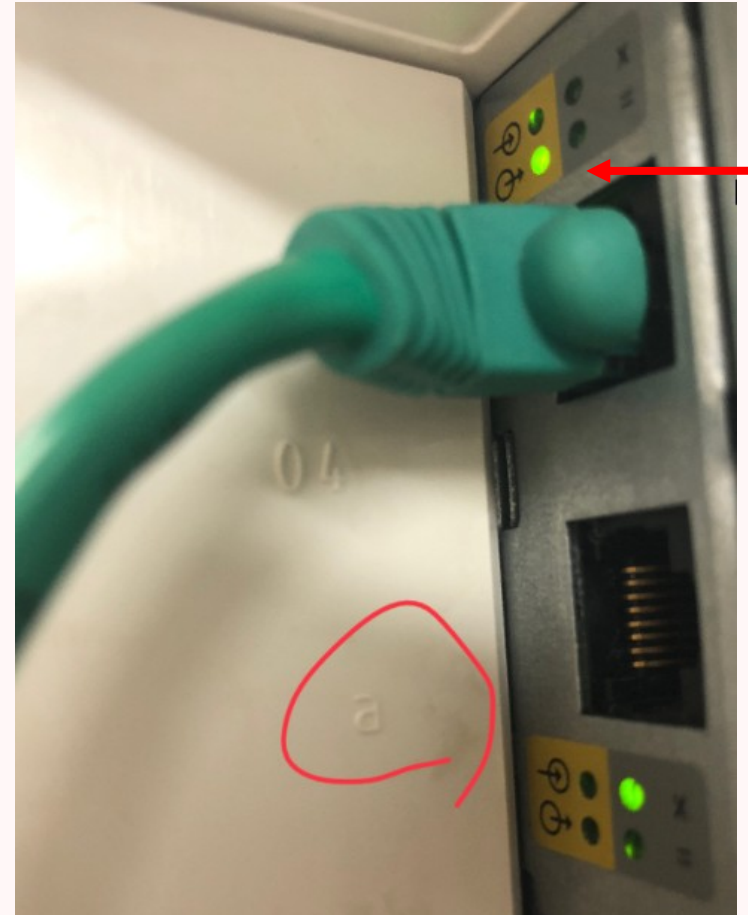

Here we are using 04b


Configuration: Philips MP70 (MIB)

- Set MIB to Yellow Arrow Out
(Device Communication Controller)
 - Go to Service mode with password: 1345
 - Select Main Setup
 - Select Hardware
 - Select Interface
 - Select Set the port (04a or 04b) to DtOut1

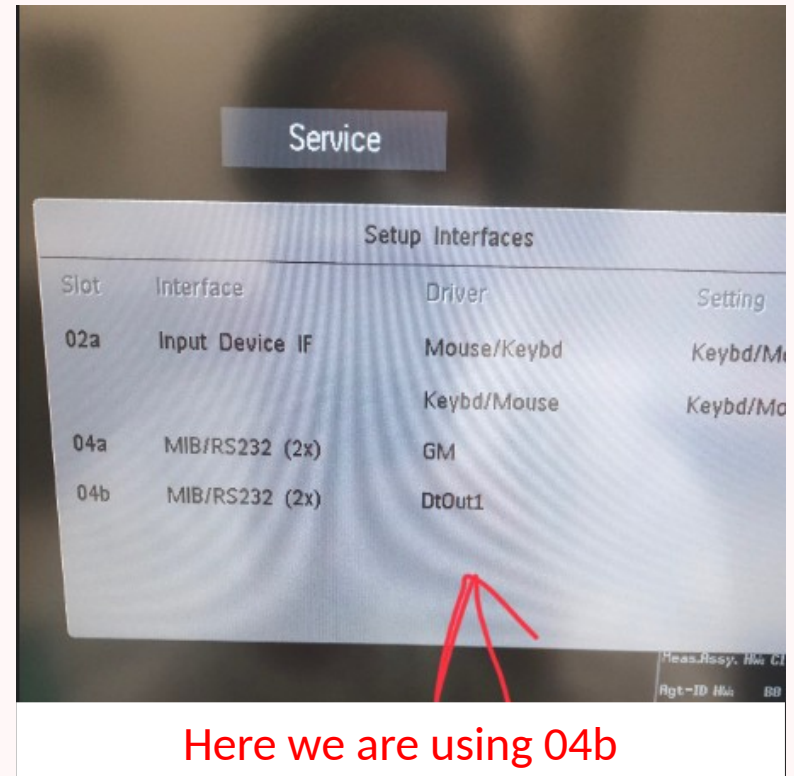

Configuration: Philips MP70 (MIB)

- Setting the Data Export
 - Baud Rate = 115200
- Select Main Setup
 - Select Setup Hardware
 - Select Data Export 1 if using DtOut1
 - Set 115200

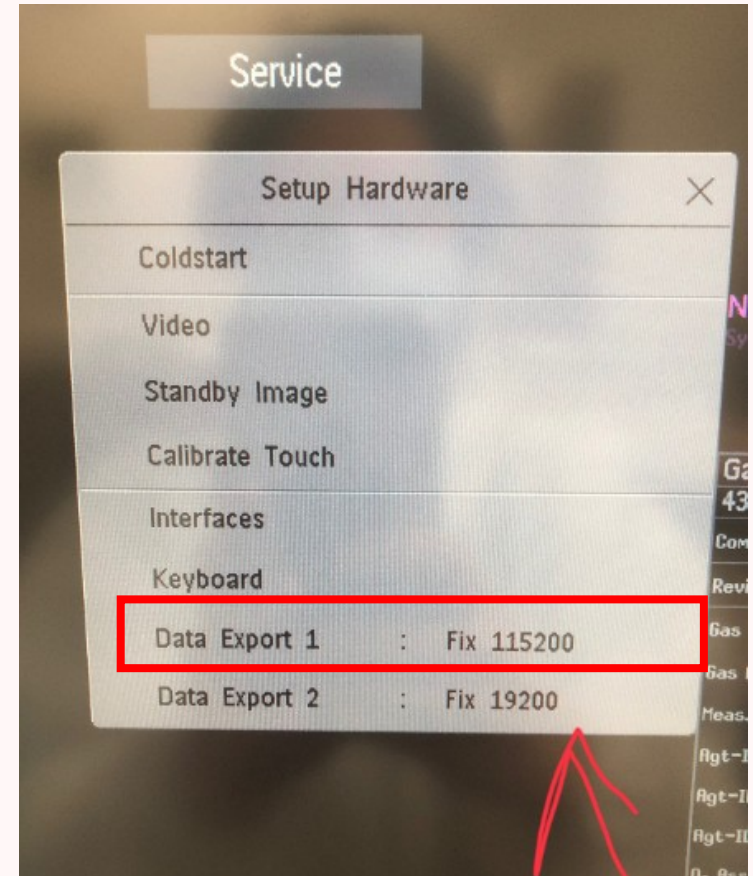

Here we are using Data Export 1

Information: Philips MP70

- Default Password for Philips
 - Config - 71034
 - Service - 1345
 - Demo - 14432

Configuration: GE Avance


- None



Optional: QR Tag

If the package contains a QR Tag, affix it to a visible location on the medical devices. Users scan the QR Tag to pick up the vital sign data.

WARNING: The QR Tag has a Nexi Name, which must match the Nexi on the medical devices all the time. A mismatch would lead to pulling wrong data.

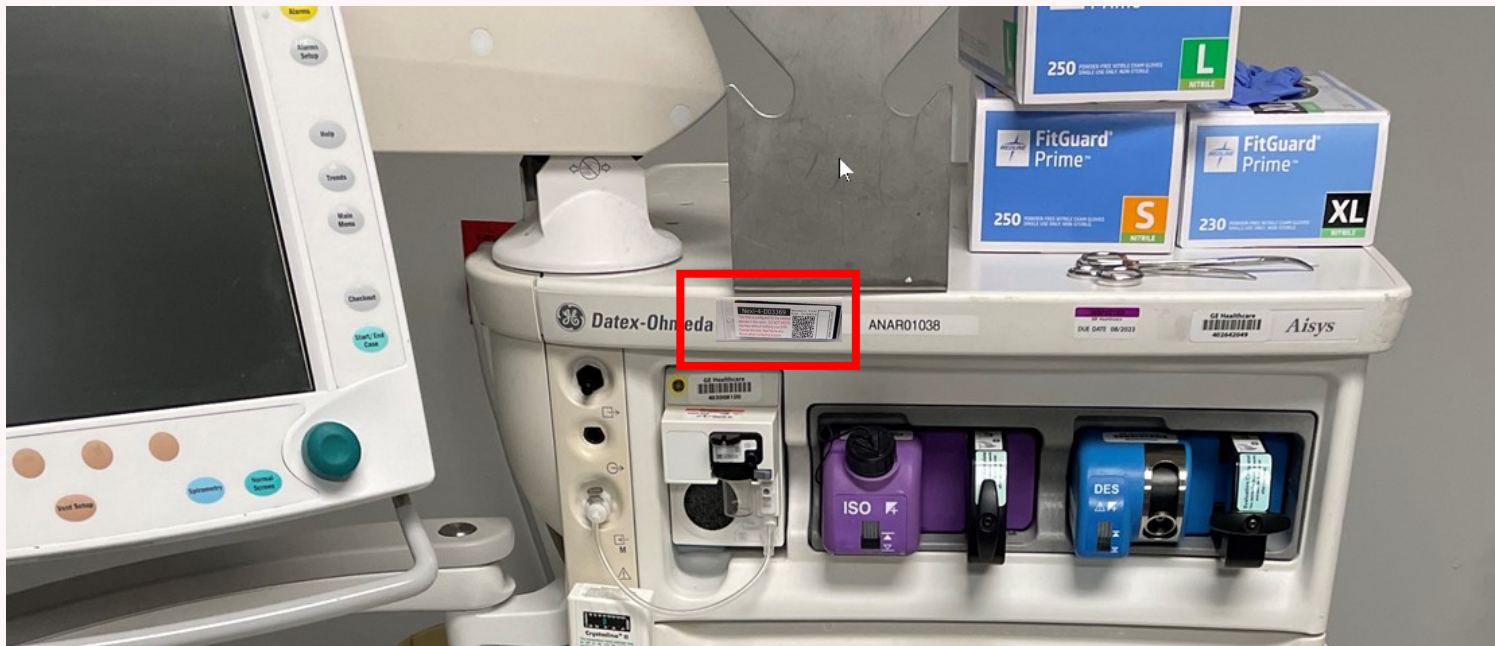


Testing: Nexi-6

- Post installation check

- Nexi is properly mounted
- Power connection to the Nexi
- Cable connection between the Nexi and medical devices
- Medical device settings if specified
- Network cable connection if using Ethernet
- All cables and cord are properly managed

- Observe

- Power light should be solid green.
- Network light should be solid green.
- Server light should be solid green.
- Data Transmission may blink blue.

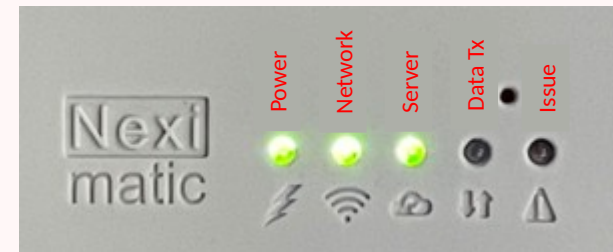

Testing: Nexi-6


■ Testing

- Turn on the medical devices
- Put a Pulse Ox sensor on you
- When measurements are on the medical devices, scan the QR code on the Nexi and follow the instruction to review the live vital sign data.




Information: Nexi-6

- Starting a reboot sequence.

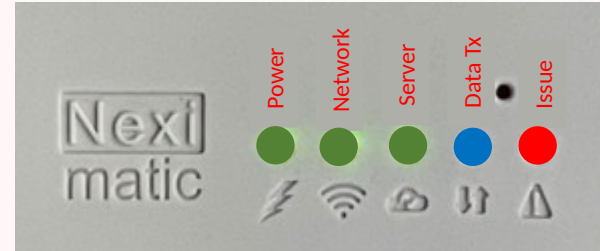


- During a reboot sequence.
- When the blue light goes off, operation begins.

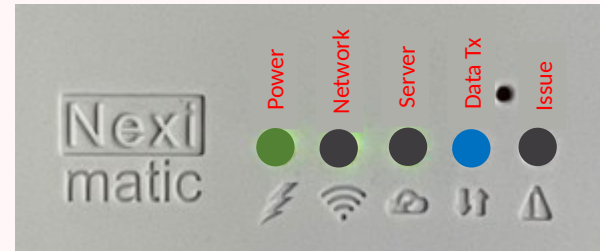


Information: Nexi-6


- Operation begins and Power light stays on.

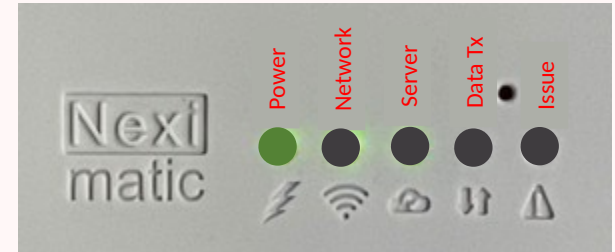

- Regardless of WIFI or Ethernet, when there is a network connection, the Network light goes green.

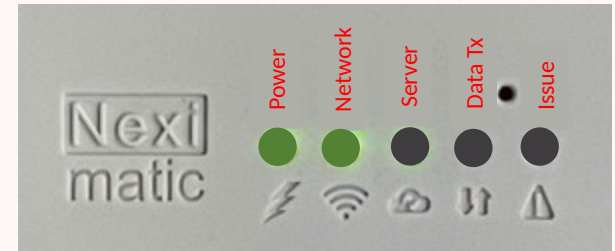

- When the Nexi can reach its server, the Server light goes on green. This Server light has to be on.

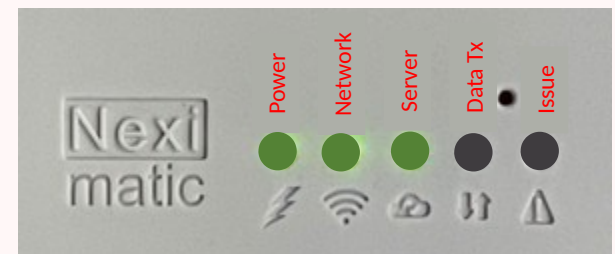

Information: Nexi-6

- When there is any issue the Issue light goes on red. The Nexi would attempt a sequence of recovery. The recovery may involve a reboot.

